






1

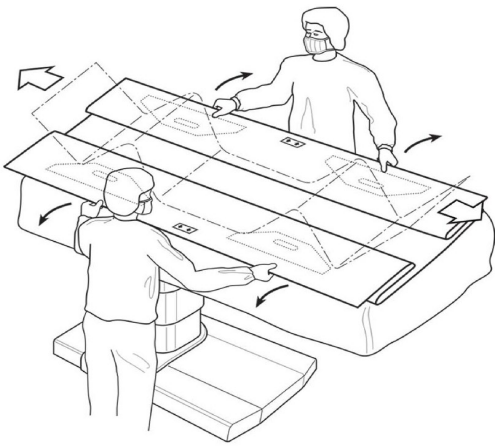


2

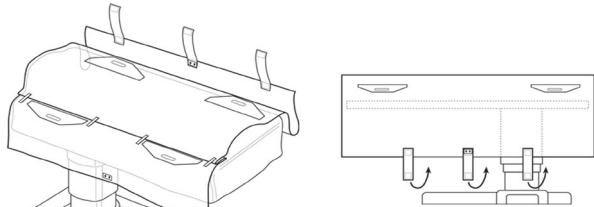


3

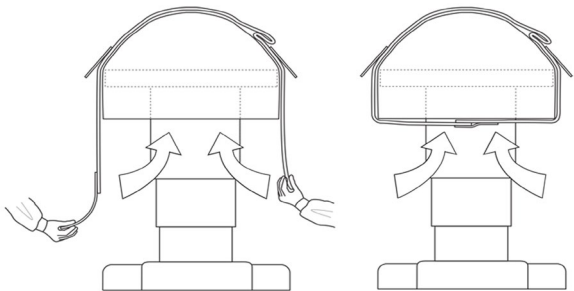


4

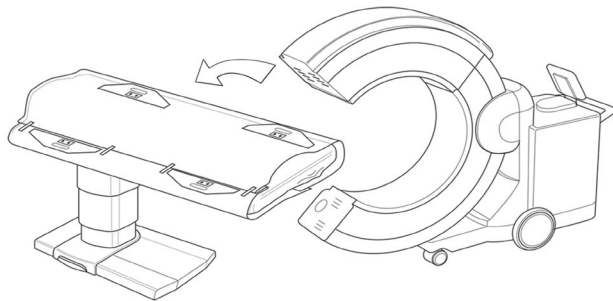


5

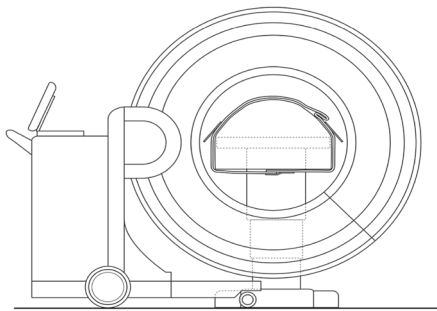


6

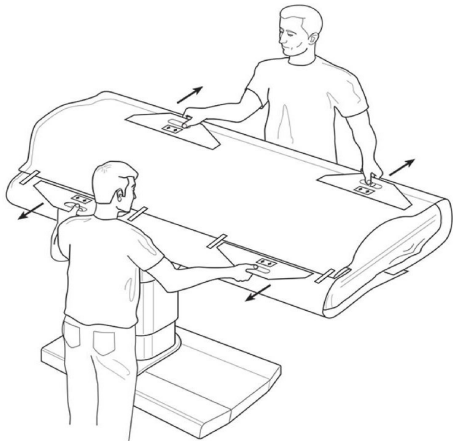

7

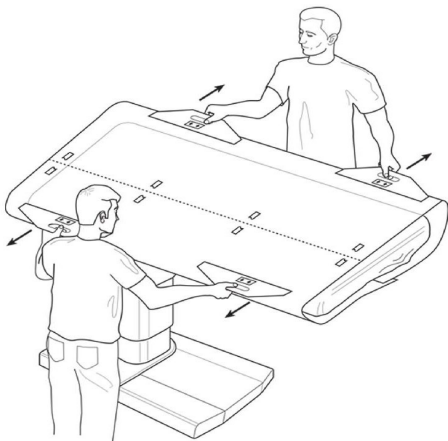

8

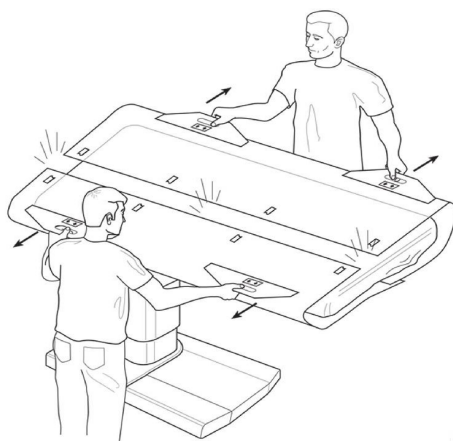

9

STERILE-Z™

REF 5574

Catalog Number

QTY 1

Quantity

LOT 1234567890

Batch Code

STERILEEO

Sterilized using ethylene oxide

 2009-01-22

Date of Manufacture

 2014-01-22

Use By Date

PACKAGE MUST BE ASEPTICALLY OPENED

 **CONTENTS STERILE UNLESS SEAL IS BROKEN OR PACKAGE IS PUNCTURED**

 Do Not Re-Sterilize

 Do Not Re-use

 Not Made With Natural Rubber Latex

 Contains No PVC

 See Instructions

EC REP Authorized representative in the European Community

EC Regulatory Matters:
MDSS GmbH Schiffgraben 41
D-30175 Hannover, Germany

CE 2797

Manufactured By:
TIDI Products, LLC
570 Enterprise Drive
Neenah, WI 54956 USA
1.800.521.1314 +1.920.751.4300
www.tidiproducs.com

For US and Foreign patent information,
See go.tidiproducs.com/patents

USA Rx Only Caution:
Federal law restricts this
device to sale by or on the
order of a Physician

EN – STERILE-Z™ Patient Drape Intended For Use With: Surgical Patient

FR – Sterile-Z™ Patient Drapé
Conçu pour être utilisé avec: Chirurgicaux Patient
DE – Sterile-Z™ Patient Abdecktuch
Für die Verwendung mit: Chirurgischen Patient
IT – Sterile-Z™ Paziente Drappo
Previsto per l'uso con: Paziente Chirurgico
ES – Sterile-Z™ Paciente Drape
Pensado para uso con: Paciente Quirúrgico
PTBR – Sterile-Z™ Paciente Drape
Intencional For Uso Com: Cirúrgico Paciente
ZH – Sterile-Z™病人垂感
擬用於同：的外科病人
JA – Sterile-Z™患者ドレーブ
と一緒に使用することを意図した：外科患者
BG – Sterile-Z™ за пациента покривка
Предназначени за използване с: Хирургично за пациента
zh – Sterile-Z™病人披覆
擬用于同：的外科病人
HR – Sterile-Z™ Pacijent Ogrnuti
Namijenjen za uporabu s: Kirurški Pacijent
CS – Sterile-Z™ Pacienta Rouška
Určen pro použití s: Chirurgická Pacienta
DA – Sterile-Z™ Patient Drapere
Beregnet til brug med: Kirurgiske Patient
NL – Sterile-Z™ Patiënt Drape
Bedoeld voor gebruik met: Operatiepatiënt
ET – Sterile-Z™, Patsiendi Laotama
Mõeldud kasutamiseks koos: Kirurgilise Patsiendi
FI – Sterile-Z™ Potilas Drape
Tarkoitettu käytettäväksi kanssa: Kirurginen Potilas
EL – Sterile-Z™ Ασθενούς Drape
Προορίζεται για χρήση με: Χειρουργικού Ασθενούς
HU – Sterile-Z™, Beteg Drape
Történő használatra tervezett -val: Sebészeti Beteg
KO – Sterile-Z™환자 드레이프
함께 사용하도록되어 있습니다: 수술 적 환자
LV – Sterile-Z™ Pacienta Drapēt
Paredzēts lietošanai ar: Kirurgiskās Pacienta
LT – Sterile-Z™ Paciento Uždangalas
Skirtas naudoti su: Chirurginės Paciento
NO – Sterile-Z™ Pasient Drape
Beregnet for bruk med: Kirurgisk Pasient
PL – Sterile-Z™ Pacjenta Drape
Przeznaczony użytku w połączeniu z: Chirurgiczne Pacjenta
PT – Sterile-Z™ Paciente Drape
Projetado para uso com: Paciente Cirúrgico
RO – Sterile-Z™ Pacientul Drape
Proiectat pentru utilizare cu: Pacientul Chirurgical
RU – Sterile-Z™ Пациента Пелерина
Предназначен для использования с: Хирургическая Пациента
SR – Sterile-Z™ Пацијент Драпе
Намњен за употребу са: Хируршки Пацијент
ID – Sterile-Z™ Pasien Drape
Ditujukan Untuk Gunakan Dengan: Surgical Pasien
SK – Sterile-Z™ Pacienta Růško
Určeny pre použitie s: Chirurgická Pacienta
SL – Sterile-Z™ Bolnik Ogrnuti
Namenjena za uporabo z: Kirurške Bolnik
SV – Sterile-Z™ Patient Drape
Avsedd att användas med: Kirurgisk Patient
TR – Sterile-Z™ Hasta Drape
Yönelik kullanim için ile: Cerrahi Hasta
UK – Sterile-Z™ пацієнта драпірувати
Призначений для використання з: хірургічне пацієнта

California's "Prop 65" law requires the following statement on many medical devices, even though they are properly processed per all current FDA and international standards: Warning: this product contains a chemical known to the state of California to cause cancer, birth defects or other reproductive harm (trace residuals from EtO sterilization).

Made in: CHINA

5574-300-005